

## pH/O.R.P. probe



- For many different types of installations and applications
- Large selection of probe for a wide range of holder
- Useable for pipe DN15 to DN200

Type 8203 can be combined with...



**Type 8200**

Probe holder



**Type 8200**

Probe holder to install in Type S020 Fitting



**Type 8619**

multiCELL transmitter/controller



**Type 8202**

ELEMENT pH/O.R.P. meter



**Type 8202**

ELEMENT neutrino pH/O.R.P. meter

The pH or O.R.P. Bürkert meter is a modular device designed for the measurement of:

- the pH in clean liquids or liquids containing solids, sulphides or proteins.
- the oxidation-reduction potential in clean liquids or liquids containing solids, sulphides or proteins which may present low conductivity.

The probes of Type 8203 are available in various models:

- for pH
  - Type PLASTRODE pH 120 mm
  - Type FLATRODE pH 120 mm
  - Type LOGOTRODE pH 120 mm
  - Type UNITRODE PLUS pH 120 mm
  - Type CERATRODE pH 120 mm
  - Type FERMTRODE VP pH 120 mm
- for O.R.P.
  - Type FLATRODE O.R.P 120 mm
  - Type LOGOTRODE O.R.P 120 mm
  - Type UNITRODE PLUS O.R.P 120 mm

### General data

#### Measuring range

Bürkert pH probe  
Bürkert O.R.P. probe

0... 14 pH  
-2000 mV... +2000 mV

#### Medium temperature

Temperature limits may depend on the inserted probe. Refer to the relevant instruction manual or technical data on next page. If the temperature ranges given for the holder and the inserted probe are different, use the most restrictive range.

#### Medium pressure

Pressure limits may depend on the inserted probe. Refer to the relevant instruction manual or technical data on next page. If the pressure ranges given for the holder and the inserted probe are different, use the most restrictive range.

#### Temperature compensation (option for pH measurement)

automatic (integrated Pt100 or Pt1000) or manual compensation reference temperature 25°C (77°F)

#### Electrical connection

Coaxial shielded cables with connector for pH/O.R.P. and 4-wire cable for Pt1000/Liquid earth rod

### Electrical data

#### Output

Analog signal, to be connected to ELEMENT or ELEMENT neutrino pH/O.R.P. meter Type 8202 or multi-CELL transmitter/controller Type 8619

### Environment

#### Ambient temperature

Temperature limits may depend on the inserted probe. Refer to the relevant instruction manual or technical data on next page for more details

## pH probe - specific technical data

Probe	PLASTRODE pH 120	FLATRODE pH 120	LOGOTRODE pH 120
<b>Medium</b>	- cost effective probe for drinking water, aquarium, swimming-pool...	- Contaminated (viscous, suspended solids, small sized solids, paints, cosmetics, foodstuffs)	- Clean (drinking water, cooling-water, aquarium, swimming-pool...)
<b>Measuring range</b>	0... 14 pH	0... 14 pH	0... 14 pH
<b>Medium pressure</b>	0 - 6 bar (0 - 87 PSI)	0 - 6 bar (0 - 87 PSI)	0 - 6 bar (0 - 87 PSI)
<b>Medium temperature</b>	-10°C to +40°C (14°F to 104°F)	0°C to +80°C (32°F to 176°F)	-10°C to +60°C (14°F to 140°F)
<b>Ambient temperature</b>			
Operation	0°C to +60°C (32°F to 140°F)	0°C to +60°C (32°F to 140°F)	0°C to +60°C (32°F to 140°F)
Storage	4°C to +30°C (39.2°F to 86°F)	4°C to +30°C (39.2°F to 86°F)	4°C to +30°C (39.2°F to 86°F)
<b>Minimal conductivity</b>	50 µS/cm	50 µS/cm	2 µS/cm
<b>Max. pressure at max. temperature</b>	6 bar (87 PSI)	4 bar (58 PSI)	6 bar (87 PSI)
<b>No. of diaphragms</b>	1	1	1
<b>Diaphragm</b>	"single pore™"	Annular and centered, in High Density Polyethylen	"single pore™"
<b>Reference electrolyte</b>	polymer	Acrylamide gel KNO <sub>3</sub> /3.5M KCl-AgCl	polymer
<b>EHEDG</b>	No	No	No
<b>Temperature sensor</b>	No	No	No
<b>Electrical connector</b>	S7/S8	S7/S8	S7/S8

	UNITRODE PLUS pH 120	CERATRODE pH 120	FERMTRUDE pH 120
<b>Medium</b>	- Contaminated (waste water, cooling water, electroplating, paints, cosmetics...) - containing sulfides/proteins (tannery, animal breeding, waste water, foodstuffs, cosmetics, biotechnology)	- High pressure, high flowrate applications	biotechnology, pharma, food industry - containing proteins, cell cultures, injectable - applications requiring biocompatibility or suitability for food contact guarantee
<b>Measuring range</b>	0... 14 pH	0... 14 pH	0... 14 pH
<b>Medium pressure</b>	0 - 16 bar if medium temperature < +100°C (0 - 232 PSI if medium temperature < 212°F) 0 - 10 bar if medium temperature between 100°C and +130°C (0 - 145 PSI if medium temperature between 212°F and 266°F)	0 - 16 bar at 25°C (0 - 232 PSI at 77°F) 0 - 6 bar at 130°C (0 - 87 PSI at 266°F)	0 - 6 bar (0 - 87 PSI)
<b>Medium temperature</b>	0°C to +130°C (32°F to 266°F)	0°C to +130°C (32°F to 266°F)	0°C to +140°C (32°F to 284°F)
<b>Ambient temperature</b>			
Operation	0°C to +60°C (32°F to 140°F)	0°C to +60°C (32°F to 140°F)	0°C to +60°C (32°F to 140°F)
Storage	4°C to +30°C (39.2°F to 86°F)	4°C to +30°C (39.2°F to 86°F)	4°C to +30°C (39.2°F to 86°F)
<b>Minimal conductivity</b>	2 µS/cm	50 µS/cm	100 µS/cm
<b>Max. pressure at max. temperature</b>	6 bar (87 PSI)	6 bar (87 PSI)	6 bar (87 PSI)
<b>No. of diaphragms</b>	2	3	1
<b>Diaphragm</b>	"single pore™"	HP ceramics	HP-COATRAMIC
<b>Reference electrolyte</b>	polymer	gel	Pressurized FOODLYTE
<b>EHEDG</b>	No	No	Yes
<b>Temperature sensor</b>	No	No	Yes, Pt100
<b>Electrical connector</b>	S7/S8	S7/S8	VP 6.0 multipin connector

## O.R.P. probe - specific technical data


Probe	FLATRODE O.R.P. 120	LOGOTRODE O.R.P. 120	UNITRODE PLUS O.R.P. 120
<b>Medium</b>	- Contaminated (viscous, suspended solids, small sized solids, paints, cosmetics, foodstuffs)	- Clean liquids (cooling-water, waste water or slightly contaminated) - with low conductivity (pure or rainwater...>2 $\mu\text{S/cm}$ )	- Clean liquids (drinking water, aquarium, swimming-pool...) - Contaminated (waste water, cooling water, electroplating, paints...) - with low conductivity (pure or rainwater...>2 $\mu\text{S/cm}$ ) - containing sulfides/proteins (tannery, animal breeding, waste water, foodstuffs, cosmetics, biotechnology...)
<b>Measuring range</b>	-2000... +2000 mV	-2000... +2000 mV	-2000... +2000 mV
<b>Medium pressure</b>	0 - 6 bar (0 - 87 PSI)	0 - 6 bar (0 - 87 PSI)	0 - 16 bar if medium temperature < +100°C (0 - 232 PSI if medium temperature < 212°F) 0 - 10 bar if medium temperature between 100°C and +130°C (0 - 145 PSI if medium temperature between 212°F and 266°F)
<b>Medium temperature</b>	0°C to +80°C (32°F to 176°F)	-10°C to +60°C (14°F to 140°F)	0°C to +130°C (32°F to 266°F)
<b>Ambient temperature</b>			
Operation	0°C to +60°C (32°F to 140°F)	0°C to +60°C (32°F to 140°F)	0°C to +60°C (32°F to 140°F)
Storage	4°C to +30°C (39.2°F to 86°F)	4°C to +30°C (39.2°F to 86°F)	4°C to +30°C (39.2°F to 86°F)
<b>Minimal conductivity</b>	50 $\mu\text{S/cm}$	2 $\mu\text{S/cm}$	2 $\mu\text{S/cm}$
<b>Max. pressure at max. temperature</b>	4 bar (58 PSI)	6 bar (87 PSI)	6 bar (87 PSI)
<b>No. of diaphragms</b>	1	1	2
<b>Diaphragm</b>	Annular and centered, in High Density Polyethylen	"single pore™"	"single pore™"
<b>Reference electrolyte</b>	Acrylamide gel $\text{KNO}_3/3.5\text{M KCl-AgCl}$	polymer	polymer
<b>EHEDG</b>	No	No	No
<b>Temperature sensor</b>	No	No	No
<b>Electrical connector</b>	S7/S8	S7/S8	S7/S8

## Principle of operation

The pH or redox probe built up on a glass membrane with variable sensitivity according to the pH or the redox, which must be screwed into the selected probe holder Type 8200, connected to the e.g. transmitter/controller 8619. The probe with S7/S8 electrical connector can be screwed into the pH/O.R.P. ELEMENT meter 8202 (standard or neutrino version) too. The probe must be calibrated with buffer solution before the installation of the sensor into the pipe.

- ▶ When a pH probe is immersed into the solution a difference in potential is formed due to ions (H<sup>+</sup>) between the glass membrane and the solution. This difference in potential measured in relation to a reference electrode is directly proportional to the pH value (59.16 mV per pH unit at 25°C). The pH meter can be calibrated in 1-point (Offset at pH 7) or in 2-points (Offset at pH 7 and Span at pH 4 or pH 10).
- ▶ When a redox probe is immersed into the solution an ion exchange occurs between the oxidised and the reduced state of an electrolyte. The generated cell voltage is the oxidation-reduction potential value. The O.R.P. meter can only be calibrated in 1-point (Offset).

## Installation of the sensor




The device has to be installed with a maximum angle of 75 degrees against the vertical onto an horizontal pipe. Select and install the required fitting onto the pipe, according to specific requirements of the device and fitting material (temperature and pressure). After having connected the device to the Type 8619 (pH/O.R.P.) multiCELL transmitter/controller and having calibrated the unit, cautiously install the complete pH/O.R.P. meter on the fitting.

In order to get reliable measurement air bubbles must be avoided.

**Please ensure that the mounting location provides a continuous and complete immersion of the probe in the flow stream.**

The probe must continuously be immersed into the measuring fluid in order to protect it from drying out. The device must be protected from constant heat radiation and other environmental influences, such as direct exposure to sunlight.

Dimensions [mm]

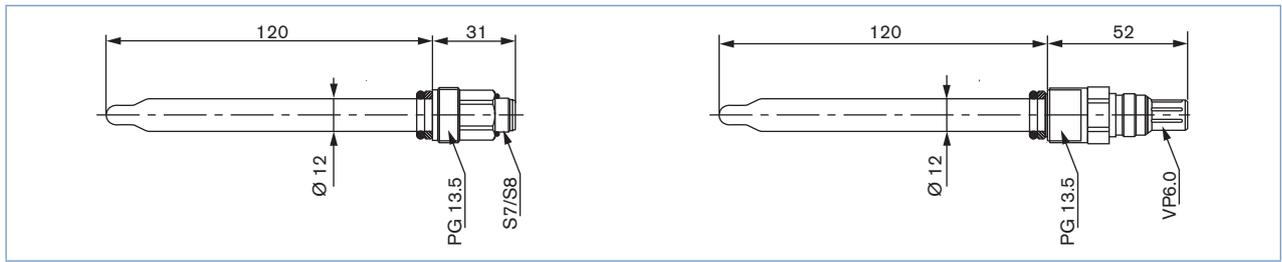

Ordering information for complete pH/O.R.P. sensor


A complete pH/O.R.P. sensor consists of a pH or O.R.P. probe Type 8203, a Pt1000/liquid earth rod (option), a probes holder Type 8200 with seals, a pH/O.R.P. shielded cable, a Pt1000/liquid earth rod shielded cable (option).

The following information is necessary for the selection of a complete device:

- **Item no.** of the desired probes holder **Type 8200** (see separate data sheet [More info.](#))
- **Item no.** of the selected pH or O.R.P. probe **Type 8203** (see ordering chart, p. 5)
- **Item no.** of the Pt1000/liquid earth rod, if needed (see ordering chart, p. 5)
- **Item no.** of the pH/O.R.P. shielded cable (see ordering chart, p. 5)
- **Item no.** of the Pt1000/liquid earth rod shielded cable, if needed (see ordering chart, p. 5)

When you click on the orange box "More info.", you will come to our website for the resp. product where you can download the data sheet.

→ You have to order the components separately.

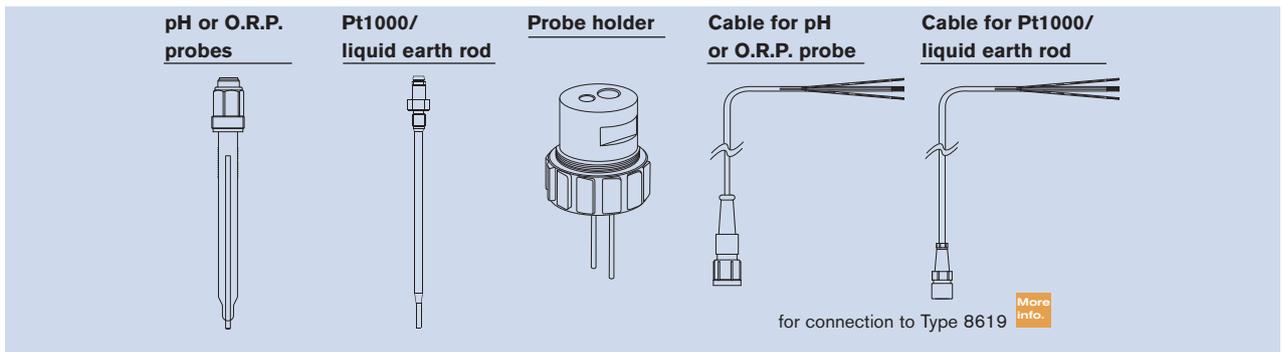

Ordering information for complete pH/O.R.P. meter


A complete pH/O.R.P. meter consists of a replaceable standard 120 mm pH or O.R.P. probe Type 8203 and a pH or O.R.P. meter Type 8202.

The following information is necessary for the selection of a complete device:

- **Item no.** of the selected pH or O.R.P. probe **Type 8203** (see ordering chart, p. 5)
- **Item no.** of the selected pH/O.R.P. meter **Type 8202** (see separate data sheet [More info.](#))

When you click on the orange box "More info.", you will come to our website for the resp. product where you can download the data sheet.

→ You have to order the components separately.

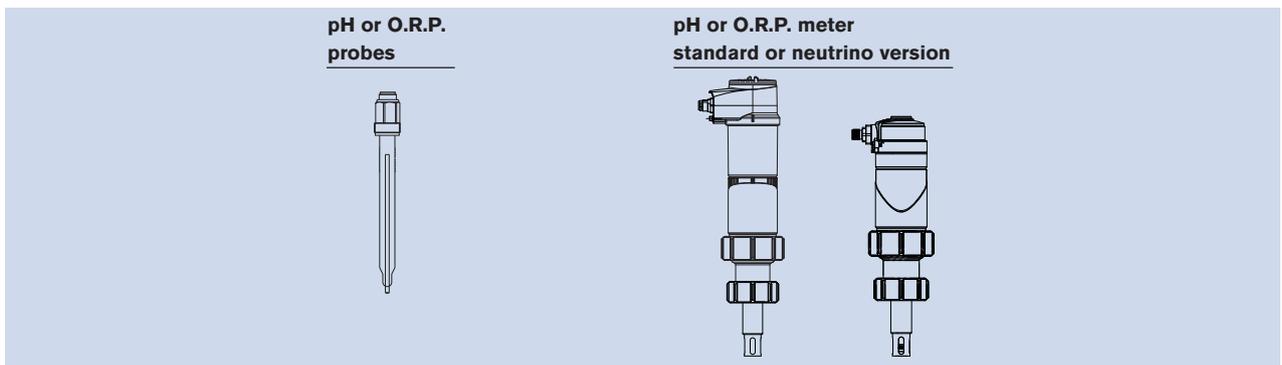

## Ordering chart for probe

Probe	Description	Item no.
<b>PLASTRODE pH 120 mm</b>	pH probe -10... 40°C, 0... 6 bar, pH 0... 14	560 377
<b>FLATRODE pH 120 mm</b>	pH probe 0... 80°C, 0... 6 bar, pH 0... 14	561 025
<b>LOGOTRODE pH 120 mm</b>	pH probe -10... 60°C, 0... 6 bar, pH 0... 14	427 114
<b>UNITRODE PLUS pH 120 mm</b>	pH probe 0... 130°C, 0... 16 bar, pH 0... 14	560 376
<b>CERATRODE pH 120 mm</b>	pH probe 0... 130°C, 0... 16 bar, pH 0... 14	418 319
<b>FERMTRODE pH 120 mm</b>	pH probe 0... 140°C, 0... 6 bar, pH 0... 14	561 727

Probe	Description	Item no.
<b>FLATRODE O.R.P. 120 mm</b>	O.R.P. probe 0... 80°C, 0... 6 bar, -2000... +2000 mV	561 027
<b>LOGOTRODE O.R.P. 120 mm</b>	O.R.P. probe -10... 60°C, 0... 6 bar, -2000... +2000 mV	560 379
<b>UNITRODE PLUS O.R.P. 120 mm</b>	O.R.P. probe 0... 130°C, 0... 16 bar, -2000... +2000 mV	560 378

Probe	Description	Item no.
Temperature probe	Pt1000/liquid earth rod - in stainless steel	427 023
Temperature probe	Pt1000/liquid earth rod - in titanium	560 317


## Ordering chart for cables for probes

Description	Item no.
pH/O.R.P. coaxial cable with standard probe plug - 3 m (for connection between 8619 transmitter and pH/O.R.P. probe mounting into Type 8200)	561 904
pH/O.R.P. coaxial cable with standard probe plug - 5 m (for connection between 8619 transmitter and pH/O.R.P. probe mounting into Type 8200)	561 905
pH/O.R.P. coaxial cable with standard probe plug - 10 m (for connection between 8619 transmitter and pH/O.R.P. probe mounting into Type 8200)	561 906
pH/O.R.P. cable with VarioPin (VP 6.0) probe plug - 3 meters (for connection between 8619 transmitter and pH/O.R.P. probe mounting into Type 8200)	554 855
pH/O.R.P. cable with VarioPin (VP 6.0) probe plug - 5 meters (for connection between 8619 transmitter and pH/O.R.P. probe mounting into Type 8200)	554 856
pH/O.R.P. cable with VarioPin (VP 6.0) probe plug - 10 meters (for connection between 8619 transmitter and pH/O.R.P. probe mounting into Type 8200)	554 857
Pt1000/liquid earth rod 4-wire cable with M8 connector - 2 m (for connection between 8619 transmitter and Pt1000/liquid earth rod mounting into Type 8200)	427 110
Pt1000/liquid earth rod 4-wire cable with M8 connector - 3 m (for connection between 8619 transmitter and Pt1000/liquid earth rod mounting into Type 8200)	561 907
Pt1000/liquid earth rod 4-wire cable with M8 connector - 5 m (for connection between 8619 transmitter and Pt1000/liquid earth rod mounting into Type 8200)	427 113
Pt1000/liquid earth rod 4-wire cable with M8 connector - 10 m (for connection between 8619 transmitter and Pt1000/liquid earth rod mounting into Type 8200)	554 822
Pt1000/liquid earth rod 4-wire cable with plug-in connector - 5 m (for connection between 8619 transmitter and Pt1000/liquid earth rod mounting into the immersion fitting Type 8200)	562 627
Pt1000/liquid earth rod 4-wire cable with plug-in connector - 10 m (for connection between 8619 transmitter and Pt1000/liquid earth rod mounting into the immersion fitting Type 8200)	562 628

## Ordering chart for accessories

Description	Item no.
Storage solution for probe (KCl 3M), 500 ml	418 557
Cleaning solution set for probe, 3 x 500 ml	560 949
Buffer solution, 500 ml, pH = 4.01	418 540
Buffer solution, 500 ml, pH = 7	418 541
Buffer solution, 500 ml, pH = 10.01	418 543
Buffer solution, 500 ml, O.R.P. = 475 mV	418 555
Factory 2-point pH calibration certificate	550 673
Factory 1-point O.R.P. calibration certificate	550 674

## Interconnection possibilities with other Bürkert devices

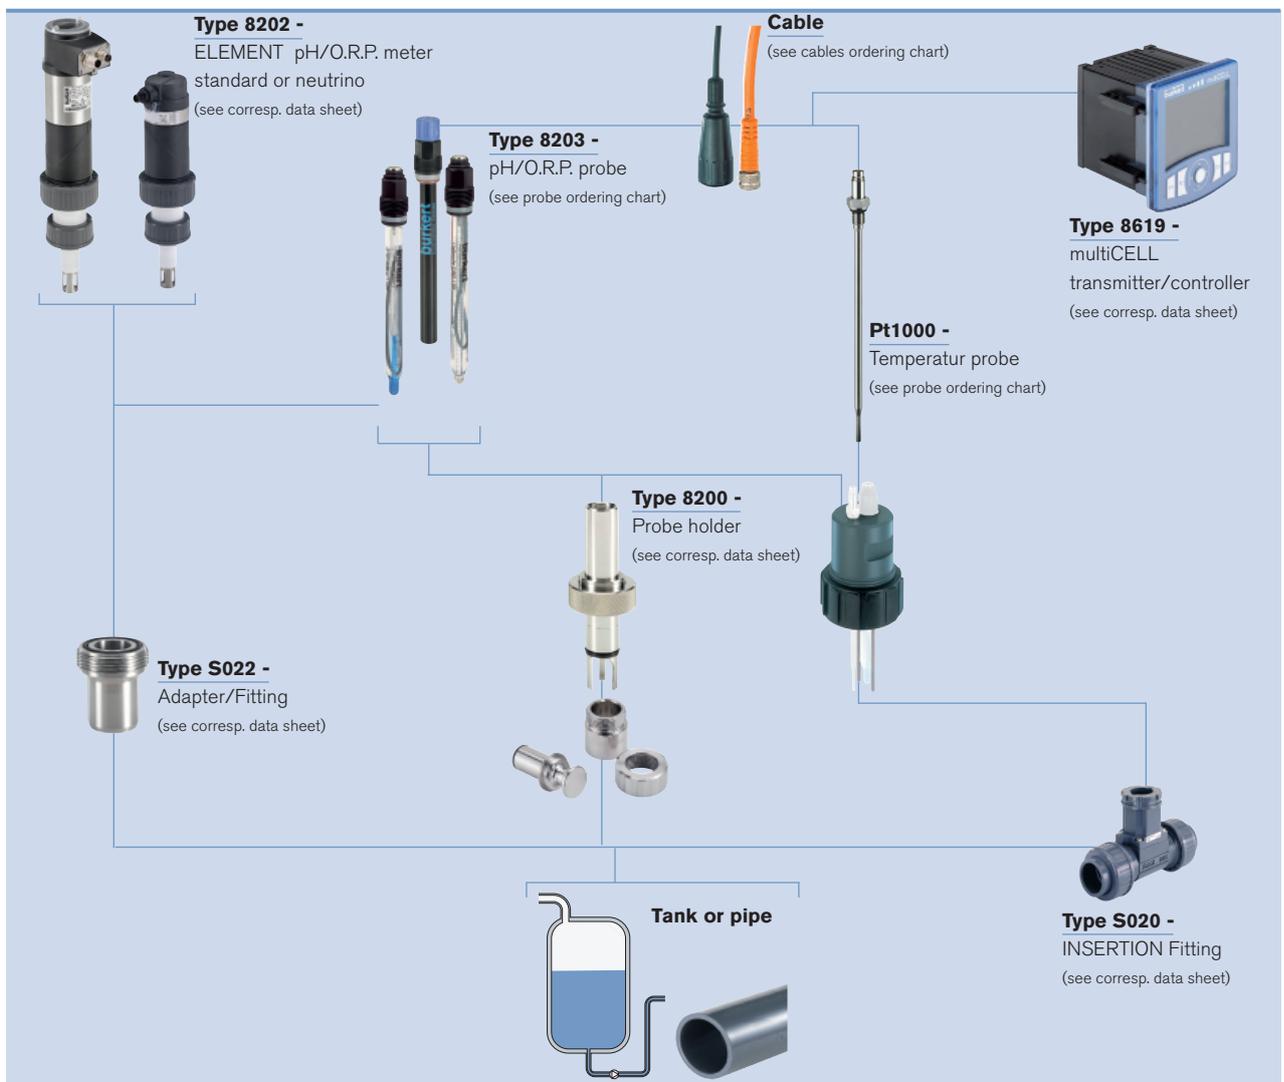

To find your nearest Bürkert office, click on the orange box →

[www.burkert.com](http://www.burkert.com)In case of special application conditions,  
please consult for advice.Subject to alteration.  
© Christian Bürkert GmbH & Co. KG

1402/6\_EU-en\_00895193